



Rhombic 3D Condylar Fracture Plate


Three-dimensional geometries
for multilateral forces



Oral and maxillo-facial surgery is our passion!
Its further development, together with our
customers, is our ambition. Every day we work
on developing innovative products and services
which meet the highest demands on quality,
and which contribute to the wellbeing of
the patient.

Rhombic 3D Condylar Fracture Plate

Three-dimensional geometries for multilateral forces

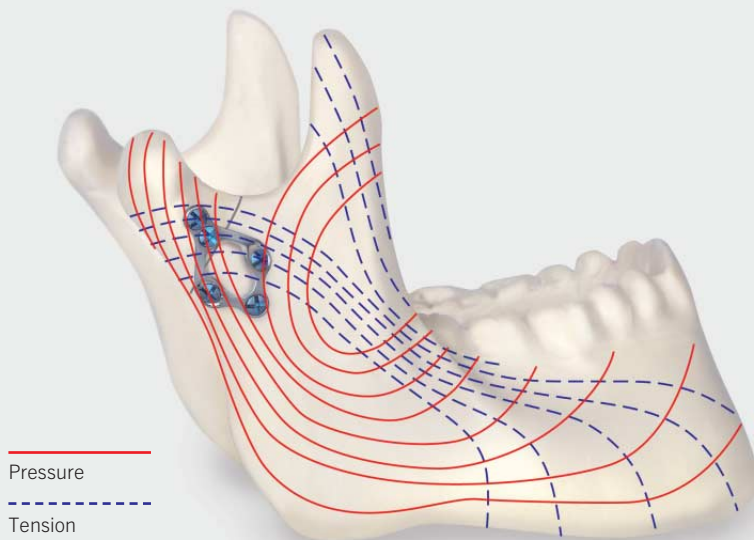

Developed in collaboration with

Prof. Dr. Dr. Günter Lauer,
University Hospital of Dresden

Pattern of the tensile and pressure forces present in the mandible. The special geometry of the Rhombic 3D Condylar Fracture Plate ensures optimal force transmission.

Rhombic 3D Condylar Fracture Plate

Condylar fractures surely are among the greatest challenges with which surgeons can be confronted in the region of the craniomaxillofacial skeleton. The considerable degree of dislocation, the lack of working space and the proximity to vital vessels and nerve structures are inherent aspects that make many physicians recoil from any surgical treatment of such conditions. However, more recent studies have shown that a generally better aesthetic and functional result can be achieved by careful open surgery using the best possible approach. Moreover, the range of available osteosynthesis materials (micro- and mini-plates, meshes, resorbable solutions, etc.) is so wide that surgeons frequently find it hard to make their choices. With the Rhombic 3D Condylar Fracture Plate, KLS Martin offers you a medium that is perfectly adapted to the multilateral masticatory forces present in this area.

Advantages

- The rhombic shape of the plate takes account of the great variety of pressure and tensile forces involved in the masticatory process, thus ensuring rigid, torsionresistant osteosynthesis.
- Thanks to the rhomboidal lightweight design, the plate provides a central window for perfect control of the fracture gap after reduction.
- Closely positioned screw holes in the cranial part of the plate allow you to place the osteosynthesis screws securely even where space is very limited.

Indications

- Surgical treatment of deep, medium and high condylar fractures

Contraindications

- Diacapitular fractures

Approaches


- Intraoral approach and endoscopically assisted intraoral approach
- Preauricular or auricular approach, especially in the case of high condylar fractures
- Periangular approach
- Retromandibular approach
- Retroauricular approach
- Submandibular approach


Note


The narrow side of the implant is fixed in place cranially (top), the wide base must be placed caudally (bottom).

The plates are available in two different versions:

Icon explanations

 Pure titanium



 Plate profile



 Items/pack

STERILE  Sterile packed implants




1/1

25-285-05-09  

25-285-05-71  



20 x 13 mm



 = 1.0 mm

Standard version (non-locking)





1/1

25-283-05-09  

25-283-05-71  

20 x 13 mm

 = 1.0 mm



Locking version

Fixation by

- 2.0-mm Mini osteosynthesis screws, non-locking
- 2.3-mm Fracture osteosynthesis screws, non-locking
- 2.0-mm ThreadLock TS locking screws (angle-stable)
- 2.3-mm ThreadLock TS locking screws (angle-stable)
- 2.0-mm Mini osteosynthesis screws, non-locking
- 2.3-mm Fracture osteosynthesis screws, non-locking

Special properties

- Special gliding holes allow raising the condyle securely to its original position
- The locking plate (green anodization) is usually implanted with locking (angle-stable) osteosynthesis screws from the 2.0/2.3-mm ThreadLock TS system. This gives you a maximum lateral range of angulation of 40° (± 20° in every direction).
- The locking feature keeps the screw exactly in the chosen angulation relative to the osteosynthesis medium. This provides a self-supporting structure that prevents resorption caused by pressing the bone against the plate when tightening the screws.
- Alternatively, it is also possible to use non-locking screws from the 2.0 Mini and 2.3 Fracture standard osteosynthesis product lines. These screws offer the advantage of a significantly wider range of lateral angulation compared to the locking screws. Of course, the locking effect will not be available in this case.

Illustrations



The procedure step by step using the standard version for illustration

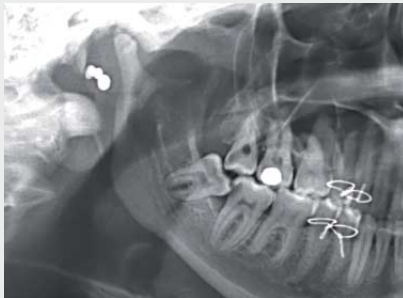


Fig. 1: Preoperative X-ray of the condylar fracture



Fig. 2: Since condylar fractures are almost always dislocated fractures, the surgeon usually will start by placing the osteosynthesis screw ❶ next to the fracture gap on the fractured condyle, because this hole is easily accessible. This is followed by inserting the second osteosynthesis screw ❷ located cranially to the first screw.



Fig. 3: Now the plate is securely fixed to the fractured bone segment. Following intra-operative verification of the anatomically correct position of the condyle or proximal fragment, this position can be secured step by step by inserting additional screws in the intact, distal region of the mandible. The special gliding hole geometry ensures that there is still a gliding range of 2.5 mm left for further corrections or adjustments.



Fig. 4: The final osteosynthesis screw is inserted as soon as the fracture has been well repositioned. This screw neutralizes the gliding hole effect.



Fig. 5: Postoperative X-ray

Case example: Treatment of a bilateral condylar fracture using the locking version



Fig. 1: Preoperative X-ray



Fig. 2: Endoscopically assisted intraoral approach to expose the condylar fracture. The fracture is visibly dislocated.



Fig. 3: Using a hooklet, it was possible to raise the fractured bone segment and restore it to its original position, thus correcting the dislocation.



Fig. 4: Important advantage of the Rhombic 3D Condylar Fracture Plate: the fracture is easily visible through the window of the plate. This gives the surgeon perfect control.



Fig. 5: Postoperative X-ray

Ordering data



1/1

25-285-05-09 **Ti** 1

25-285-05-71 **Ti** 1

20 x 13 mm

1.0 mm




1/1

25-283-05-09 **Ti** 1

25-283-05-71 **Ti** 1

20 x 13 mm

1.0 mm



Icon explanations

Ti Pure titanium

Plate profile

1 Items/pack

STERILE IR Sterile packed implants

References

- Haim, D., et al.,
Biomechanical study of the Delta Plate
and the TriLock Delta Condyle Trauma Plate.
J Oral Maxillofac Surg, 69 (10), 2011,
S. 2619 – 2625
- Lauer, G.,
Condylar neck fractures: Delta-shaped plate
and endoscopic approach. In:
Haerle, F., et al., Atlas of craniomaxillofacial
osteosynthesis. 2. Auflage, Thieme Verlag,
Stuttgart, New York, 2009, S. 78 – 84
- Lauer, G., et al.,
A new 3-dimensional plate for transoral
endoscopic-assisted osteosynthesis of
condylar neck fractures.
J Oral Maxillofac Surg, 65 (5), 2007,
S. 964 – 971
- Lauer, G., et al.,
Plate osteosynthesis of the mandibular condyle.
Ann Anat, 189 (4), 2007, S. 412 – 417
- Lauer, G., et al.,
Transoral osteosynthesis of condylar neck
fractures using a three-dimensional plate.
Mund-Kiefer-Gesichtschir, 10 (5), 2006,
S. 335 – 340
- Lauer, G. & Schmelzeisen, R.,
Endoscope-assisted fixation of mandibular
condylar process fractures.
J Oral Maxillofac Surg, 57 (1), 1999, S. 36 – 40
- Schmelzeisen, R., et al.,
Endoscope-assisted fixation of condylar
fractures of the mandible.
Mund-Kiefer-Gesichtschir, 1998 May,
2 Suppl 1, S. 168 – 170
- Schneider, M., et al.,
Surgical treatment of fractures of the mandible
condyle: a comparison of long-term results
following different approaches – functional,
axiographical, and radiological findings.
J Craniomaxillofac Surg, 35 (3), 2007,
S. 151 – 160

Brochures



Osteosynthesis 2.0 Mini



Osteosynthesis 2.3
Fracture and Reconstruction



ThreadLock TS
Osteosynthesis 2.0 - 2.7
Fracture and Reconstruction



Instruments for treating
condylar fractures



Angulus2
angled screwdriver

KLS Martin Group

KLS Martin Australia Pty Ltd.

Sydney · Australia
Tel. +61 2 9439 5316
australia@klsmartin.com

KLS Martin do Brasil Ltda.

São Paulo · Brazil
Tel. +55 11 3554 2299
brazil@klsmartin.com

KLS Martin Medical (Shanghai) International Trading Co., Ltd.

Shanghai · China
Tel. +86 21 5820 6251
china@klsmartin.com

KLS Martin India Pvt Ltd.

Chennai · India
Tel. +91 44 66 442 300
india@klsmartin.com

Martin Italia S.r.l.

Milan · Italy
Tel. +39 039 605 67 31
italia@klsmartin.com

Nippon Martin K.K.

Tokyo · Japan
Tel. +81 3 3814 1431
nippon@klsmartin.com

KLS Martin SE Asia Sdn. Bhd.

Penang · Malaysia
Tel. +604 505 7838
malaysia@klsmartin.com

Martin Nederland/Marned B.V.

Huizen · The Netherlands
Tel. +31 35 523 45 38
nederland@klsmartin.com

Gebrüder Martin GmbH & Co. KG

Moscow · Russia
Tel. +7 499 792-76-19
russia@klsmartin.com

Gebrüder Martin GmbH & Co. KG

Dubai · United Arab Emirates
Tel. +971 4 454 16 55
middleeast@klsmartin.com

KLS Martin UK Ltd.

London · United Kingdom
Tel. +44 1189 000 570
uk@klsmartin.com

KLS Martin LP

Jacksonville · Florida, USA
Tel. +1 904 641 77 46
usa@klsmartin.com

Gebrüder Martin GmbH & Co. KG

A company of the KLS Martin Group

KLS Martin Platz 1 · 78532 Tuttlingen · Germany
P.O. Box 60 · 78501 Tuttlingen · Germany
Tel. +49 7461 706-0 · Fax +49 7461 706-193
info@klsmartin.com · www.klsmartin.com

